



UvA-DARE (Digital Academic Repository)

Computer Assisted Centrifugal Elutriation. I

Detection system and data acquisition equipment

Sloot, P.M.A.; Carels, M.J.; Tensen, P.; Figdor, C.G.

DOI

[10.1016/0169-2607\(87\)90030-7](https://doi.org/10.1016/0169-2607(87)90030-7)

Publication date

1987

Document Version

Final published version

Published in

Computer Methods and Programs in Biomedicine

[Link to publication](#)

Citation for published version (APA):

Sloot, P. M. A., Carels, M. J., Tensen, P., & Figdor, C. G. (1987). Computer Assisted Centrifugal Elutriation. I: Detection system and data acquisition equipment. *Computer Methods and Programs in Biomedicine*, 24(3), 179-188. [https://doi.org/10.1016/0169-2607\(87\)90030-7](https://doi.org/10.1016/0169-2607(87)90030-7)

General rights

It is not permitted to download or to forward/distribute the text or part of it without the consent of the author(s) and/or copyright holder(s), other than for strictly personal, individual use, unless the work is under an open content license (like Creative Commons).

Disclaimer/Complaints regulations

If you believe that digital publication of certain material infringes any of your rights or (privacy) interests, please let the Library know, stating your reasons. In case of a legitimate complaint, the Library will make the material inaccessible and/or remove it from the website. Please Ask the Library: <https://uba.uva.nl/en/contact>, or a letter to: Library of the University of Amsterdam, Secretariat, P.O. Box 19185, 1000 GD Amsterdam, The Netherlands. You will be contacted as soon as possible.

CPB 00831

Computer-assisted centrifugal elutriation. I. Detection system and data acquisition equipment

P.M.A. Sloot¹, M.J. Carels², P. Tensen¹ and C.G. Figdor¹

¹ Division of Biophysics and Immunology, The Netherlands Cancer Institute and ² Computer Science Department, University of Amsterdam, Amsterdam, The Netherlands.

To optimize cell separations by centrifugal elutriation, we constructed an on-line computer-controlled multiparametric light-scatter system. A bypass sample flow, at the outlet of an elutriation rotor, is hydrofocussed and three scatter parameters of each cell are determined up to a maximum of 15000 cells/second. The 18-bit representation of the parameter values are cumulatively stored by means of a direct memory access interface. The histogram memory is continuously displayed to provide information on the number and type of cells that are elutriated. A special purpose operating system, implemented on a stand-alone computer configuration, allows a high data-acquisition rate and ample data processing capacity. In addition, a local network driver was constructed to facilitate off-line detailed analysis of the data. The equipment is well suited to monitor the centrifugal elutriation process. The flexibility of the system allows an extension of the monitor to computer-controlled elutriation.

Cell separation; Centrifugal elutriation; Multiparametric light-scatter analysis; Stand-alone computer; Operating system; Local network

1. Introduction

Centrifugal elutriation (CE) is a powerful physical cell separation technique by means of which differences in sedimentation velocity of human peripheral blood cells are exploited to isolate various types of cells [1–3]. It is well suited for separating large numbers of mononuclear cells into lymphocytes and monocytes [4–7], or isolating subpopulations of monocytes that differ in function and maturation/differentiation stage [8]. Currently, CE is widely used to purify inhomogeneous cell populations, for both clinical and fundamental research

applications [8–10]. However, until now separations have been carried out in a rather arbitrary manner, since analysis of elutriated cells is performed after separation. Therefore two major disadvantages are related to the practical application of CE.

First, during elutriation no information is present on the progress of the separation process. This implies that optimization of the CE technique can only be attained by means of trial-and-error methods [11–14]. Secondly, the morphological differentiation and characterization of the various eluted fractions is an extremely time-consuming process, thus limiting the practical applicability of CE. Cell identification equipment, with a data acquisition unit, interfaced to the CE rotor might overcome these disadvantages. However, since CE is generally applied to prepare homogeneous cell populations for further biological ex-

Correspondence P.M.A. Sloot, Division of Biophysics and Immunology, The Netherlands Cancer Institute, Antoni van Leeuwenhoek Huis, Plesmanlaan 121, 1066 CX Amsterdam, The Netherlands.

periments, no biochemical modification (e.g. staining) of the cells under separation is allowed. This implies that we are limited to nondestructive remote sensing of cells that emerge from the rotor.

The present communication reports on the construction of an on-line real-time computer-controlled light-scatter apparatus to monitor and optimize cell separations performed by CE. A separate paper describes the off-line software developed to analyze the data available from elutriation experiments. This equipment allows on-line monitoring of the separation process and instant analysis of the isolated fractions.

2. Background

In this section, a concise description of the CE technique, as well as a brief review of the elastic light-scatter properties of a single cell in flow, is presented. Concurrently, the disadvantages related to CE, and the considerations with respect to the design of the detection system, are discussed.

In CE—or counterflow centrifugation—a fluid is pumped into the center of a centrifuge rotor through a rotating seal. The fluid moves through internal tubing into a divergent chamber situated in the rotor. At the end of this chamber the flow reconverges into a small tube and leaves the system through the rotating seal. As described previously, concentration of the cells is accomplished by means of a second rotor in series with the first one [15]. A mononuclear cell suspension, prepared by a blood component separator [16], is injected into the first rotor and moves through the system into the separation chamber. The separation chamber coerces the cells to rest, relative to the rotor, at a point where the outward-directed centrifugal forces are balanced by the inward-directed fluid dynamics. The cell population redistributes itself along the separation chamber in accordance with the physical properties (volume and density) of each cell (Fig. 1) [1–3,17]. Fractionation is obtained by stepwise decreases of the speed of the first rotor, while the speed of the second rotor remains at a constant value to collect and concentrate the eluted cells. Further details of the CE equipment, the sample introduction and

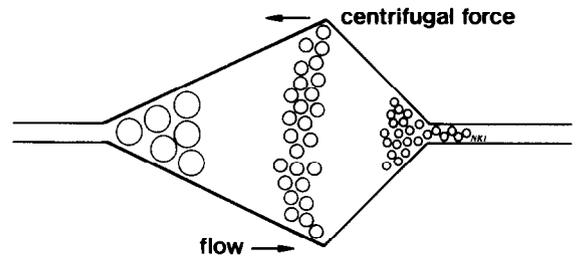


Fig. 1. Redistribution of mononuclear cells in a centrifugal elutriation rotor chamber.

the flow distribution unit were described previously [15].

Inherent in the CE technique are several factors that might influence the resolution capacity of the cell separation. Optimization of the CE system is obtained by investigating these resolution-improving parameters. For instance, the influence of temperature of the fluid [11,12,14], the shape of the elutriation chamber [14,17] and cell load and density of the elutriation fluid [18], were studied and modified to optimize the separation process. Morphological characterization of the fractions is always performed after separation by staining the cytocentrifuge preparations and by electronic sizing. This implies that no information is available during the separation process. In addition, the differentiation is hampered by subjective interpretation (microscopic analysis), or poor differentiation capacity (electronic sizing cannot always discriminate between various subpopulations of human blood cells). An on-line detection system will improve the interpretation of this type of experiment. Such a system reveals information on the characteristics of the separation process, and reliable fractionation criteria (e.g. fractionation time and speed of the rotor) are within reach.

In a previous investigation, Mulder et al. constructed a one-parameter monitor to study the purification of monocytes by means of CE [19]. Although this monitor could not discriminate between the various (sub)populations (e.g. monocytes/granulocytes), and did not allow further analysis of the data, the results clearly demonstrated the applicability of such a monitor system. Therefore we designed a light-scatter device, interfaced to the CE system, which facilitates detection

of all significant subpopulations in human peripheral blood. Most light-scatter instruments (e.g. flow cytometers) used for the differentiation of biological cells, measure forward scatter (FS) vs. fluorescence or FS vs. side scatter (SS) [20–24]. Recently, however, we showed numerically that optimization of the detection can be obtained by the simultaneous measurement of FS, SS and back scatter (BS) [25]. Therefore, a three-parameter light-scatter monitor was designed and interfaced to the CE system.

3. Design considerations

In the previous sections we emphasized the necessity of an on-line three-parametric light-scatter apparatus to monitor CE experiments. The equipment should meet certain specific conditions, which are discussed in this section.

Table 1 shows the statistics of a typical CE experiment in which mononuclear cells, isolated from peripheral blood of a human donor, are separated under standard conditions. Morphological characterization of the fractionated populations is established by May Grünwald Giemsa staining of cytocentrifuge preparations and subsequent microscopical analysis [15,16]. The data exhibit a characteristic maximum number of cells in the lymphocyte fractions (at a rotor speed of 3100 rpm). Since we are interested in the maximum number of cells *per second*, the elutriation profile of the 3100-rpm fraction is measured (by counting each minute the number of cells that are eluted from the first rotor). The results show that a new equilibrium is established within 2 min (Fig. 2). Subsequently, the cell rate slowly decreases and the nonequilibrium cells are eluted from the separation chamber. From Table 1 and Fig. 2 it can be concluded that the maximum cell rate expected is approximately 1×10^6 cells/s. Consequently, three parametric detection of a significant number of the eluted cells ($\sim 0.3\%$) necessitates a high-speed data-acquisition system.

The biological spread causes a homogeneous broadening of the light-scatter signal. Therefore, a limited (e.g. 6-bit) resolution of each parameter is sufficient to obtain a realistic representation of each detector signal.

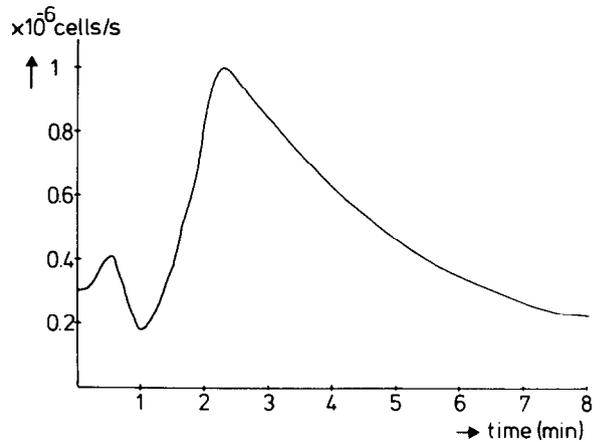


Fig. 2. Elutriation profile of a lymphocyte fraction.

On account of the large amount of data (0.3% of 10^6 cells, represented by 18 bits, equals 60 Kbits per second), a real-time histogramming direct memory access (DMA) interface has been designed. This interface imposes a memory organization where each address is defined by an 18-bit combination of the detected signal. Each new event (i.e. a detected cell) triggers the interface, and the contents of the corresponding memory location are subsequently increased by 1 (up to a maximum of $2^{16} - 1$: due to the homogeneous broadening and the total number of detected cells, the number of cells in a single channel is expected not to exceed this maximum).

Since the system should provide direct information on the elutriation process, the data, stored by means of the DMA interface, are graphically displayed on a CRT screen. To investigate the data more closely, a communication between the on-line memory and a host computer¹, is necessary. Serial transmission of the complete computer memory is too slow, since 512 Kbytes of data ($2^{18} \times 16$) results in a transfer time of almost 10 min. A parallel link, on the other hand, limits the distance between the host computer and the monitor system. To avoid these difficulties, a local area network was used. Subsequently, a network driver

¹ LoVME 68010 (Microproject BV, The Netherlands), running the Unix operating system (Unix is a trademark of Bell Labs).

TABLE 1
 Statistics of a centrifugal elutriation experiment of 700×10^6 mononuclear cells with an elutriation time of 8 min/fraction and a flow rate of 18 ml/min

Fraction	Rotor speed (rpm)	Total number of cells ($\times 10^{-6}$)	Percentage of cells in fraction			Number of cells in fraction ($\times 10^{-6}$)			Average number of cells per minute ($\times 10^{-6}$)								
			E	L	M	G	E	L	M	G	E	L	M	G			
1	3500	115	90	10				103.5	11.5				12.9	1.5			
2	3300	60	50	50				30	30				3.8	3.8			
3	3100	225	20	80				45	180				5.6	22.5			
4	3000	25	15	80	5			3.8	20	1.3			0.5	2.5	0.2		
5	2900	8	3	57	35	5		0.2	4.5	2.6	0.5		0.5	0.5	0.3	0.1	
6	2900	7	3	20	72	5		0.2	1.4	5.3	0.4		0.2	0.2	0.7	0.1	
7	2800	75	3	5	90	2		2.3	3.8	67.5	1.5		0.3	0.5	8.4	0.2	
8	2700	35	3	4	86	7		1.1	1.4	30.1	2.5		0.1	0.2	3.8	0.3	
9	2650	50	3	11	47	39		1.5	5.5	23.5	19.5		0.2	0.7	2.9	2.4	
10	stop	100	3	4	11	82		3	4	11	82		0.4	0.5	1.4	10.3	

E, erythrocytes; L, lymphocytes; M, Monocytes; G, granulocytes.

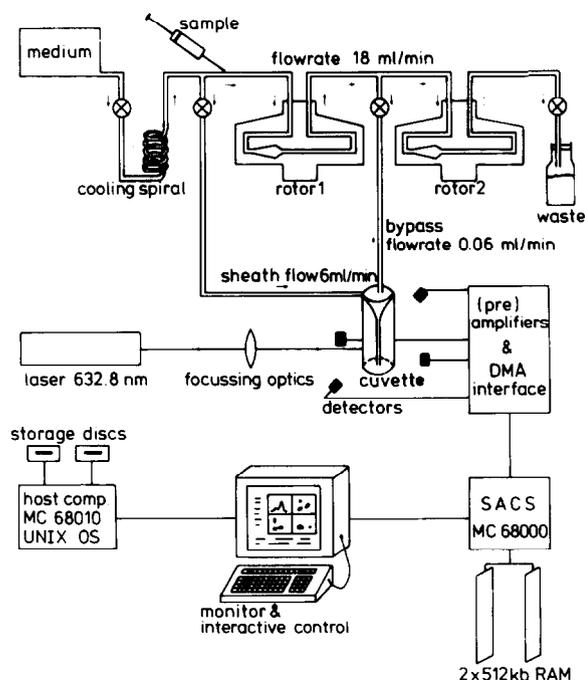


Fig. 3. Outline of the complete computer-assisted centrifugal elutriation system. SACS, stand-alone computer system; OS, operating system.

was designed and implemented. Finally, simultaneous control of data acquisition, data flow and graphical representation required a special-purpose operating system (OS). In addition, an OS (with low-level control of the hardware) allows a hardware-independent software organization. This results in flexible soft- and hardware design. Consequently, modifications and/or extensions are easily implemented.

4. System description

An outline of the complete CE monitor is shown in Fig. 3. The details of the signal processing unit and the data acquisition will be discussed in this section.

The CE system consists of two JE-6 elutriation rotors, connected in series and equipped with standard separation chambers². To monitor the

cells elutriated from rotor 1, a shunt is inserted between the two rotors. The flow rate of the bypass (0.05 ml/min) assures that a sufficient amount of elutriated cells can be studied without significantly diminishing the cell yield. The bypass sample flow is hydrofocussed into a commercially available cuvette³ to facilitate the excitation of each single cell by means of a focussed laser beam [26]. To compensate for the additional flow circuit, and the related additional flow resistance, an extra flow controller is inserted in the waste flows. This allows tuning of the combined flow system and results in a stable sample flow.

Light from a He/Ne laser⁴ is focussed by means of two crossed cylindrical lenses ($f=60$ mm and $f=20$ mm) to a laser spot of approximately $20\ \mu\text{m} \times 80\ \mu\text{m}$. The small deviation of the laser spot from the theoretical values ($15\ \mu\text{m}$ and $50\ \mu\text{m}$, respectively) is caused by inevitable misalignment and irregularities in the beam-shaping optics, but does not affect the optical detection [27]. The He/Ne excitation wavelength (632.8 nm) assures that no relevant absorption is present in the studied samples [28–30]; therefore, the light attenuation is completely described by elastic light scatter [20]. The light scattered by each cell that enters the laser field is detected in the FS, SS and BS directions by a number of photovoltaic detectors⁵. A second SS detector is installed to compensate for possible variations in the hydrofocussed sample flow. The four BS detectors (2×5 mm) are centered around the incident laser beam. The light collecting angles are: FS, 1° to 7° ; SS, 75° to 100° ; BS, 160° to 180° , respectively. The geometry of the light-scatter detectors, in combination with the related acceptance angles, guarantee optimal detection of the light-scatter parameters of nucleated blood cells: FS is sensitive to cellular gross size, SS is mainly determined by the optical density of the cytoplasm and BS is exclusively related to the optical density of the nucleus [24,25].

The scatter signals of each cell are digitized to

² Beckman Instruments, Palo Alto, CA, U.S.A.

³ Ortho Diagnostic Systems, Belgium.

⁴ 10 mW random polarized; Spectraphysics.

⁵ FS: huv-1000bq; SS: huv-4000b; EG&G; BS: 4 BPY-11 detectors (Siemens) in series.

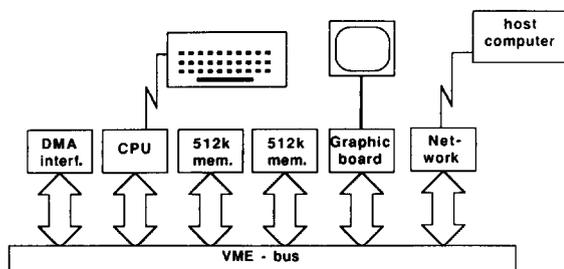


Fig. 4. Hardware configuration of the CACE equipment.

form a combined 18-bit address. By means of DMA, the contents of the address are increased by 1. This data acquisition technique is in contrast with regular techniques, where list mode facilities have been applied to detect and store multiparameter information [31]. The advantages of the simultaneous storage technique are evident: it requires only a minor on-line memory and all information (e.g. correlation between parameters), necessary for implementation of off-line parametric and non/parametric analysis [32], remains directly available. Communication between the interface, the central processor⁶, the memory⁷, the graphical board⁸ and the network adaptor⁹ is established by means of VME-bus logic (Fig. 4). In addition, cell rate, overflow occurrences and DMA activity are simultaneously measured and displayed.

To control the various processes that are active at the same time on the same processor, a time-sharing provision must be present. In addition, low-level access to various devices is necessary. Therefore, a special-purpose OS has been developed. Interrupt handling, process scheduling, device access, data manipulation as well as data representation, are controlled by this OS, the structure of which is shown in Fig. 5. The innermost (software) layer allows a process to wait for an event generated by another process, or an external event (e.g. interrupts activated by the operator). Consequently, administration of interrupts and synchronization of simultaneous processes are provided by this first layer. The

⁶ FORCE sys68K/CPU-1.

⁷ FORCE sys68K/DRAM-1.

⁸ ELTEC GRAZ-1/68K.

⁹ Microproject BV, The Netherlands, No. 2501-7969-6.

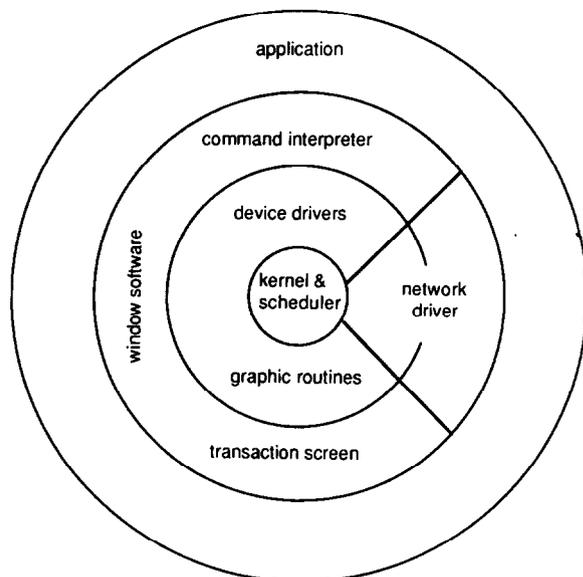


Fig. 5. Software structure of the stand-alone OS.

second layer of the OS is a uniform interface to several different hardware devices. It contains a number of procedures to perform (buffered) input and/or output (e.g. type-ahead facilities). The third layer implements the command interpreter and the (operator-computer) communication procedures. Application software, implemented as 'highest-level modules', facilitate straightforward modification and extension of the system. This stratified module structure is supported by several programming languages, e.g. ADA, PASCAL [33] and MODULA II. Since no ADA compilers were available, MODULA II was used as the most convenient language. It supports separate compilation, low-level access and has a strong modular concept. In addition MODULA II facilitates implementation of concurrent programming [34].

As described in the previous sections, elutriation is performed by decreasing the rotor speed and harvesting the eluted cells. The information of each fraction, stored in the memory, must be available for further statistical analysis. Therefore, the monitor is interfaced to a host computer by a commercially available hardware device. In the remaining part of this section we will give a concise description of the implementation of the local network on the stand-alone system.

The structure of the local network is comparable to the structure of the OS. The physical, datalink and network layers, with their corresponding protocols, are part of the standard configuration of the hard- and software of the adaptor. Implementation of a network on the OS, however, requires a transport layer (i.e. network driver) [35]. This driver resets the adaptor, reads or writes a packet, handles interrupts and closes the adaptor. In addition, the driver supports access of simultaneous processes by means of virtual devices and (de)multiplexing communication. The software constituting the dump application resides in the top layer of the network structure. It allows the operator to dump the complete updated memory to the host computer. Comparable programs exist for reading packets of information from the host computer.

The complete software package (operating system, network and application) consists of 360 Kbytes of source code. After compilation and linking, 150 Kbytes of object code remains to be downloaded.

5. Status report

The reliability of computer-assisted centrifugal elutriation (CACE¹⁰), is primarily determined by the quality of the detection system. Especially, the detection of a single cell in flow is hampered by a number of experimental difficulties. We therefore studied the performance of the light-scatter set-up by injection of various well-defined particles ($1-10 \mu\text{m} \pm 10 \text{ nm}$) into the sample flow. For instance, the influence of the beam-stop in the FS direction has been studied. Experiments showed that an extremely small beam-stop with cylindrical shape, in addition to a small detection angle, in the FS directions results in an optimal correlation between FS and particle size. This is in agreement with recent theoretical and experimental results [36]. Furthermore, it was concluded from these experiments that reflections from daylight introduce noise to the SS signal. This is due to the extreme weak SS signal: approximately 10^{-10} of

the incident radiation (i.e. $\sim 10^{-9}$ mW). Therefore, a light-screening cone was mounted onto the SS detector. In addition, a second SS detector was introduced, in series with the first one, to account for insurmountable variations in the hydro-focussed sample flow. After establishment of the quality of the detection system, the linearity of the signal amplification with respect to the frequency of particles passing through the laser beam was studied. It was concluded that a maximum cell rate of approximately 15 000 cells/s is still within the specifications of the equipment (data not shown). Since DMA signal processing is applied, the *actual* cell rate limit is also 15 kHz. This implies that the data acquisition is suitable for efficient on-line sampling (interfacing to the CE rotors).

In a preliminary software configuration, the time required to produce 4 simultaneous scatterplots exceeded 1 min. This was due to a memory-scanning module written in MODULA II. Therefore, in contrast to all the other modules, the scanning routine was rewritten in assembler code. Consequently, the current picture-producing time is as small as 15 s. Information on the CE process is therefore available within approximately 30 s (15 s additional delay is caused by the distance between the detection system and the elutriator rotor).

The merits of the network and its protocol were studied by sending and receiving a large number of 0.5-Mbyte packets. A minor adaption of the sending protocol resulted in a current (error-free) transfer time of 3.15 min for 512 kbyte of data. Since approximately 5 min are required to harvest the eluted cells from the second rotor and to initialize the next fraction, a transfer time of ~ 3 min is sufficient. However, further improvement of the speed of data transfer would contribute to the flexibility of the system (e.g. intermediate transfers). Therefore, the transfer protocols (i.e. the time-limiting modules) are still under study.

After establishment of the quality of the parts constituting the system, the equipment was assembled and interfaced to the CE rotors (Fig. 3). A number of separations were carried out to study the complete performance of the system. A flowchart representing the user-application mod-

¹⁰ Patent applied for in the Netherlands.

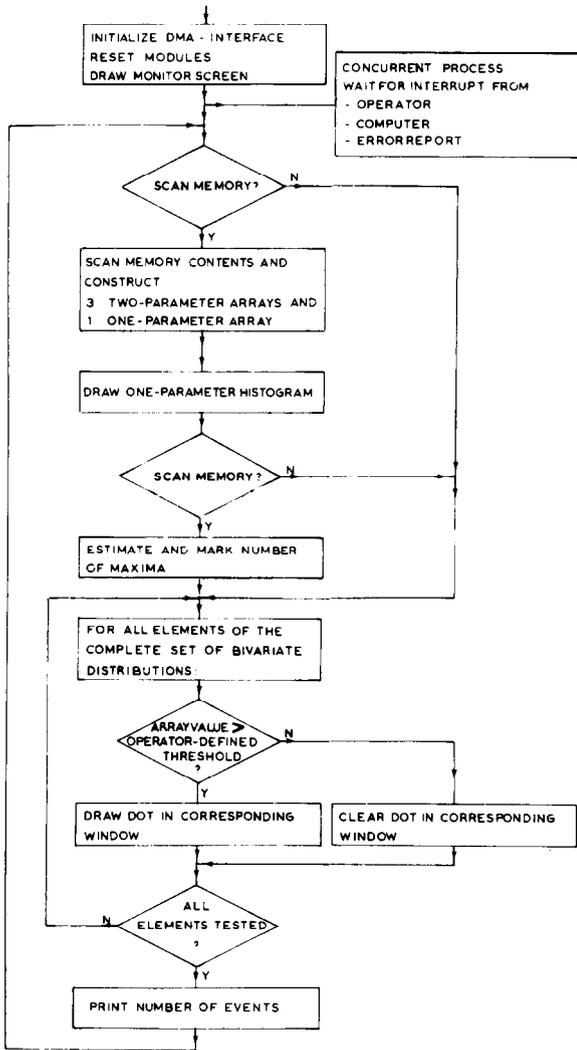


Fig. 6. Flowchart of the application module, indicating the concurrent processes during a CACE experiment.

ule is shown in Fig. 6. Two concurrent processes are active in this module: one process reads the data and calculates the information for graphical representation, whereas the other process is waiting for a computer signal or an operator signal (interrupt). The result of a typical intermediate fraction, containing lymphocytes, monocytes and a small percentage of neutrophilic granulocytes, is shown in Fig. 7. It is observed that the various (sub)populations are well defined, and that the information available from the monitor facilitates tuning of the separation process.

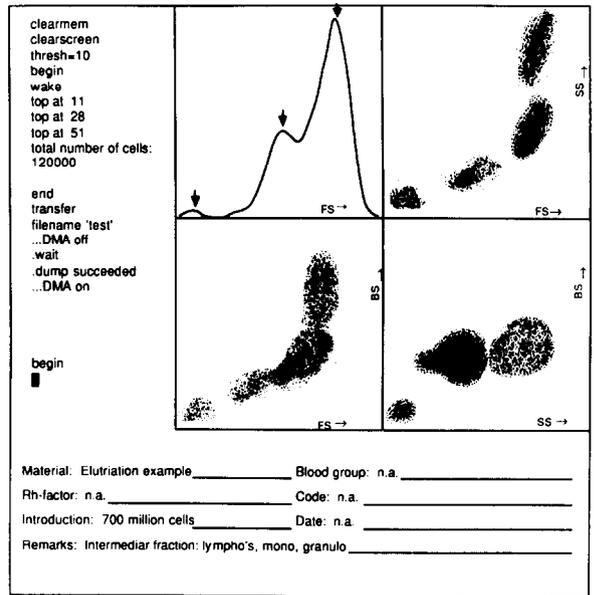


Fig. 7. A simulated screen-dump of a typical CACE experiment. The left window shows the communication of the operator with the computer. The bottom window displays the statistics of the experiment.

6. Lessons learned

In the previous sections, the necessity and the design of a CACE system is described. The current level of performance and implementation of the equipment indicates that computerized multi-parametric remote sensing of a single elutriated cell is well suited to study the CE process. The memory organization and the DMA interface allows high-speed 3-parametric data acquisition of the scatter parameters. In addition, the processor time can be used to manipulate the data, show the status of the separation process and communicate with the operator. The resolution of the scatter parameters (3 × 6 bits), assures an adequate representation of the (sub)populations of the cells that are elutriated. Higher resolution (e.g. 3 × 8 bits) will not significantly improve the scatter information. Moreover, the time required to produce an on-line scatter-plot would increase dramatically. The flexibility of this CACE system allows straightforward modification of the hardware devices and/or the user-defined software. This is

essential, since both the soft- and hardware are regularly adapted to fulfill the requirements of various types of experiments. In addition, the choice of an operating system allows a user-friendly communication between the operator and the numerous (active) processes of the computer. Therefore, the system can be applied in routine experiments such as preparative separations of a large number of human peripheral blood cells [7]. From these observations, it can be concluded that the system may facilitate both clinical and research applications.

The computer language MODULA II (a descendant of PASCAL) allows low-level access and is well suited for applications where hardware devices are interfaced. In addition, the module concept (especially the definition and implementation module facilities) and the unique procedure type facilitate the design of system software. Furthermore, compatibility and flexibility of the existing software is guaranteed by the modular structure of the software: modifications are easily implemented.

7. Conclusions and future plans

In this paper we report on the construction of a computer-assisted centrifugal elutriation device. Presently, we apply the system to investigate a number of CE parameters that could influence the resolution capacity of the separation process. For instance, the elutriation profile, the optimal elutriation time and the relation between the speed of the rotor and the separation of the various (sub)populations will be investigated. A better understanding of the fluid dynamics in the rotor chamber is within reach using this remote sensing technique. In the near future a number of modifications and/or extensions will be added to the system: to study the time-dependent inhomogeneity of an eluted fraction, intermediate dumping of the memory contents must be applied. Currently, however, the time needed for a complete data transfer is too long to allow this intermediate data transfer. Therefore, the (CRC) protocols of the network will be optimized. In addition, the top layer of the OS software will be modified to allow

more advanced graphical utilities. For instance, masked bivariate plotting capabilities and on-line software windows, to calculate changes in the eluted subpopulations, will be implemented. Downloading of the software into the stand-alone system is a time-consuming process (150 Kbytes of object code requires approximately 2 min loading time). Therefore, the complete software package will be stored into an EPROM. This allows direct execution of the software after (re)initialization of the hardware.

Recent theoretical considerations suggest that the anisotropy introduced by cellular membrane inhomogeneities and multiple scattering can be studied by measuring (de)polarization of the incident light [37,38]. The CACE system will be adapted in accordance with this observation.

The flexibility of the CACE system allows modification of the soft- and hardware to facilitate the design of a 'turn-key' computer-controlled centrifugal elutriation system. First, computer-controlled detection and regulation of the complete flow system and the rotor speed must be established. Next, an accurate on-line differentiation of the various subpopulations, and a hardware device controlling the rotor speed, must be designed. Finally, to facilitate routine application of such a system, autofocussing algorithms will be investigated [39].

Acknowledgements

We thank Drs. P.H. Hartel (University of Amsterdam) for critical reading of the manuscript, Prof. Dr. L.O. Hertzberger (University of Amsterdam) and Dr. W.S. Bont for fruitful discussions and Th. L.F.M. Helsloot (University of Amsterdam) for technical assistance.

This work was supported by the Stichting Technische Wetenschappen (STW), grant LGN-22053.

References

- [1] P.E. Lindahl, Principles of a counter streaming centrifuge for the separation of particles of different size, *Nature* London 161 (1948) 648-649.

- [2] P.E. Lindahl, On counterstreaming centrifugation in the separation of cells and cell fragments, *Biochim. Biophys. Acta* 21 (1956) 411–415.
- [3] T.G. Pretlow II and T.P. Pretlow, Centrifugal elutriation (counterstreaming and centrifugation) of cells, *Cell Biophys.* 1 (1979) 195–210.
- [4] D.A. Morris et al., Isolation of functional subsets of human peripheral blood monocytes, *J. Immunol.* 123 (1979) 166–172.
- [5] T.J. Contreras et al., An improved technique for the negative selection of large numbers of human lymphocytes and monocytes by counterflow centrifugation–elutriation, *Cell Immunol.* 54 (1980) 215–229.
- [6] R.S. Weiner and V.O. Shah, Purification of human monocytes and collection of large numbers of peripheral blood monocytes, *J. Immunol. Methods* 36 (1980) 89–97.
- [7] C.G. Figdor et al., Isolation of large numbers of highly purified lymphocytes and monocytes with a modified centrifugal elutriation technique, *J. Immunol. Methods* 40 (1981) 275–288.
- [8] C.G. Figdor et al., Isolation of functionally different human monocytes by counterflow centrifugation elutriation, *Blood* 60 (1982) 46–53.
- [9] T. de Witte et al., Bone marrow repopulation capacity after transplantation of lymphocyte-depleted allogeneic bone marrow using counterflow centrifugation, *Transplantation* 37 (1984) 151–155.
- [10] S.J. Noga et al., Large-scale separation of human bone marrow by counterflow centrifugation elutriation, *J. Immunol. Methods* 92 (1986) 211–218.
- [11] W.D. Grant and M. Morrison, Resolution of cells by centrifugation elutriation, *Analyt. Biochem.* 98 (1979) 112–115.
- [12] M.L. Meistrich and N.M. Hunter, Temperature regulation during centrifugation elutriation and its effect on cell separation, *Cell Biophys.* 3 (1981) 127–140.
- [13] P.C. Keng, C.K.N. Li and K.T. Wheeler, Characterisation of the separation properties of the Beckman Elutriation System, *Cell Biophys.* 3 (1981) 41–56.
- [14] M.L. Meistrich, Experimental factors involved in separation by centrifugation elutriation, *in: Cell separation: Methods and Selected Applications*, vol 2, eds. T.G. Pretlow II and T.P. Pretlow, pp 33–61 (Academic Press, London, New York, 1983).
- [15] C.G. Figdor et al., A centrifugal elutriation system of separating small numbers of cells, *J. Immunol. Methods* 68 (1984) 73–87.
- [16] C.G. Figdor et al., Rapid isolation of mononuclear cells from buffy coats prepared by a new blood cell separator, *J. Immunol. Methods* 55 (1982) 221–229.
- [17] R.J. Sanderson et al., Design principles for a counterflow centrifugation cell separation chamber, *Analyt. Biochem.* 76 (1976) 615–622.
- [18] C.G. Figdor et al., Theory and practice of centrifugation elutriation (CE) factors influencing the separation of human blood cells, *Cell Biophys.* 5 (1983) 105–118.
- [19] P.H.M. Mulder et al., Monocyte purification with counterflow centrifugation monitored by continuous flow cytometry, *J. Immunol. Methods* 47 (1981) 31–38.
- [20] H.C. van de Hulst, *Light Scattering by Small Particles* (Dover Publications, New York, 1981).
- [21] G.C. Salzman et al., Cell classification by laser light scattering: Identification and separation of unstained leukocytes, *Acta Cytol.* 19 (1975) 374–377.
- [22] H.M. Shapiro, Multistation multiparameter flow cytometry: a critical review and rationale, *Cytometry* 3 (1982) 227–243.
- [23] J.M. Thompson et al., The optimal application of forward and ninety degree light scatter in flow cytometry for the gating on mononuclear cells, *Cytometry* 6 (1985) 401–406.
- [24] R.A. Meyer and A. Brunsting, Light scattering from nucleated biological cells, *Biophys. J.* 15 (1975) 191–203.
- [25] P.M.A. Slood and C.G. Figdor, Elastic light scattering from nucleated blood cells: rapid numerical analysis, *Appl. Optics* 25 (1986) 3559–3565.
- [26] J.A. Steinkamp, *Flow Cytometry*, *Rev. Sci. Instrum.* 55 (1984) 1375–1400.
- [27] R.S. Longhurst, *Geometrical and physical optics* (Longman, New York, 1984).
- [28] P. Latimer et al., Changes in total light scattering and absorption caused by changes in particle conformation, *J. Theor. Biol.* 21 (1968) 348–367.
- [29] J.E. Aubin, Autofluorescence of viable cultured mammalian cells, *J. Histochem. Cytochem.* 27 (1979) 36–43.
- [30] R.C. Benson et al., Cellular autofluorescence—is it due to flavins? *J. Histochem. Cytochem.* 27 (1979) 44–48.
- [31] R.D. Hiebert and R.G. Sweet, Electronics for flow cytometers and sorters, *in: Flow Cytometry Instrumentation and Data Analysis*, eds. M.A. van Dilla, P.N. Dean, O.D. Learum and M.R. Melamed, pp. 129–162 (Academic Press, London, 1985).
- [32] R.C. Mann et al., Parametric analysis of histograms measured in flow cytometry, *Cytometry* 4 (1983) 75–82.
- [33] J.V. Cugini, *Selection and Use of General Purpose Programming Languages*, Vols. 1 and 2, *Computer Science and Technology 1984* (MBS Special Publication 500-117, LCC Nos. 84-601119 and 601120).
- [34] N. Wirth, *Programming in Modula II* (Springer Verlag, New York, 1983).
- [35] A.S. Tanenbaum, *Computer Networks* (Prentice Hall, Englewood Cliffs NJ, 1981).
- [36] P.N. Wild and J. Swithenbank, Beamstop and vignetting effects in particle size measurement by laser diffraction, *Appl. Optics* 25 (1986) 3520–3527.
- [37] S. Ziets, A. Belmont and C. Nicolini, Differential scattering of circularly polarized light as a unique probe of polynucleosome superstructures. A simulation by multiple scattering of dipoles, *Cell Biophys.* 5 (1983) 163–187.
- [38] S.R. Pal and A.I. Carswell, Polarization anisotropy in lidar multiple scattering from atmospheric clouds, *Appl. Optics* 24 (1986) 3464–3471.
- [39] F.C.A. Groen, I.T. Young and G. Lighthart, A comparison of different focus functions for use in autofocus algorithms, *Cytometry* 6 (1985) 81–91.