



UvA-DARE (Digital Academic Repository)

Transcutaneous electromyography of the diaphragm

Monitoring breathing and the effect of respiratory support in preterm infants

de Waal, C.G.

Publication date

2018

Document Version

Other version

License

Other

[Link to publication](#)

Citation for published version (APA):

de Waal, C. G. (2018). *Transcutaneous electromyography of the diaphragm: Monitoring breathing and the effect of respiratory support in preterm infants*. [Thesis, fully internal, Universiteit van Amsterdam].

General rights

It is not permitted to download or to forward/distribute the text or part of it without the consent of the author(s) and/or copyright holder(s), other than for strictly personal, individual use, unless the work is under an open content license (like Creative Commons).

Disclaimer/Complaints regulations

If you believe that digital publication of certain material infringes any of your rights or (privacy) interests, please let the Library know, stating your reasons. In case of a legitimate complaint, the Library will make the material inaccessible and/or remove it from the website. Please Ask the Library: <https://uba.uva.nl/en/contact>, or a letter to: Library of the University of Amsterdam, Secretariat, Singel 425, 1012 WP Amsterdam, The Netherlands. You will be contacted as soon as possible.

Chapter 2

Classifying apnea of prematurity by transcutaneous electromyography of the diaphragm

J.V. Kraaijenga

G.J. Hutten

C.G. de Waal

F.H. de Jongh

W. Onland

A.H. van Kaam

Neonatology 2018;113(2):140-145



Abstract

Background

Treatment of apnea is highly dependent on the type of apnea. Chest impedance (CI) has inaccuracies in monitoring respiration, which compromises accurate apnea classification. Electrical activity of the diaphragm measured by transcutaneous electromyography (EMG) is feasible in preterm infants and might improve accuracy of apnea classification.

Objectives

To compare the accuracy of apnea classification based on diaphragmatic EMG (dEMG) and CI tracings in preterm infants.

Methods

Fifteen cases of central apnea, 5 of obstructive apnea and 10 of mixed apnea were selected from recordings containing synchronized continuous tracings of respiratory inductive plethysmography (RIP), airway flow, heart rate (HR), oxygen saturation (SpO₂) and breathing activity measured by dEMG and CI. Twenty-two assessors (neonatologists, pediatricians-in-training and nurses) classified each apnea twice; once based on dEMG, HR and SpO₂ tracings, and once based on CI, HR and SpO₂. Assessors were blinded for the type of respiratory tracing (dEMG or CI) and for the RIP and flow tracings.

Results

In total 1,320 assessments were performed and in 71.1% the apnea was classified correctly. Subgroup analysis based on respiratory tracing showed that 74.8% of the dEMG tracings were classified correctly compared to 67.3% of the CI tracings ($p < 0.001$). This improved apnea classification based on dEMG was present for central (86.7% vs. 80.3%, $p < 0.02$) and obstructive (56.4% vs. 32.7%, $p < 0.001$) apnea. The improved apnea classification based on dEMG tracings was independent of the type of assessor.

Conclusion

Transcutaneous dEMG improves the accuracy of apnea classification when compared to CI in preterm infants, making this technique a promising candidate for future monitoring systems.

Introduction

Impaired control of breathing resulting in apnea is common in preterm infants with a gestational age (GA) of < 30 weeks.¹ Apnea can be classified into 3 groups: 1) central apnea, i.e. a cease in airflow due to absence of respiratory effort; 2) obstructive apnea, i.e. a cease in airflow caused by upper-airway obstruction; and 3) mixed apnea, i.e. a cease in airflow caused by a combination of both the above.^{1,2} Central and mixed apneas account for most apneic episodes.³ The frequency of apnea is inversely proportional to the GA and in almost all infants apnea is accompanied by hypoxemia and bradycardia.^{1,4}

Hypoxemic episodes, especially if prolonged, are associated with an increased risk of adverse neurodevelopmental outcome in preterm infants.⁵ Prompt and adequate treatment of apnea is therefore of the utmost importance. However, the optimal treatment of apnea is highly dependent on the type of apnea, so correct classification based on accurate cardiorespiratory monitoring is essential. For instance, central apnea is probably best treated with caffeine, while nasal continuous positive airway pressure (nCPAP) might be a better choice for obstructive apnea, as it splints the upper airway.^{6,7}

Chest impedance (CI) is the current standard for bedside cardiorespiratory monitoring of preterm infants. It measures changes in electrical impedance caused by changes in lung aeration and chest wall movement.⁸ CI provides continuous monitoring of the heart rate (HR), respiratory rate (RR) and breathing pattern; the last of these is used for detection and classification of apnea. However, CI has important limitations, such as inaccuracies in monitoring respiration due to cardiac interference and non-breathing-related chest wall movement. This may compromise accurate detection and classification of apnea.⁸⁻¹¹

Measuring electrical activity of the diaphragm might be a more direct and accurate method to monitor respiration in newborn infants. We recently showed that transcutaneous electromyography of the diaphragm (dEMG) is feasible in preterm infants and provides accurate data on HR and RR, comparable to CI.¹² No study has investigated if dEMG improves apnea classification compared to CI so far.

Therefore, the aim of this study was to compare apnea classification by CI and dEMG. We hypothesized that dEMG would allow for more accurate apnea classification than CI.

Methods

For this study, we used data collected in a previously published prospective observational cohort study conducted in the Neonatal Intensive Care Unit (NICU) of the Emma Children's Hospital, Academic Medical Center Amsterdam, the Netherlands.¹³ This study assessed the effect of caffeine on the electrical activity of the diaphragm in 30 spontaneously breathing preterm infants with a GA of < 34 weeks. All infants were

supported with nCPAP using an Infant Flow[®] or Infant Flow[®] SiPAP[™] system (Vyaire, Yorba Linda, CA, USA) or an AVEA[™] ventilator (Vyaire). Written informed consent was obtained from both parents, and the study protocol was approved by the Institutional Review Board.

In all patients, the breathing pattern measured by dEMG was recorded at the bedside using a portable 16-channel digital physiological amplifier (Dipha-16, Macawi, Enschede, the Netherlands). Two transcutaneous electrodes were placed at the costo-abdominal margin in the left and right nipple line, and 1 ground electrode at height of the sternum.¹² The averaged dEMG data were digitized without analog filtering and sent wirelessly to the front-end of the Dipha-16 system, which was connected to a personal computer. More details on pre- and post-processing, sampling rate, the filtering algorithm and other technical aspects of the dEMG measurement have been described previously.^{14,15}

In order to classify the apnea as central, obstructive, or mixed, respiratory inductance plethysmography (RIP) was used as the gold standard. Respiration was therefore also recorded with RIP, which measures rib-cage (RC) and abdominal (AB) excursions via 2 elastic bands containing a Teflon-coated wire connected to a Bicare-II device (Vyaire). An electrical oscillating signal is sent simultaneously through both wires and the frequency modulation due to expansion and contraction of the RC and AB bands is converted to voltage changes.^{16,17} The sum signal of the RC and AB bands was also calculated (summed RIP).

CI and transcutaneous oxygen saturation (SpO_2) recorded by an Intellivue MP-90 monitor (Philips Healthcare, Eindhoven, The Netherlands) were captured by a personal computer at a sample rate of 500 Hz using custom made software.

Finally, a disposable AVEA[™] Ventilator VarFlex Flow Transducer (Vyaire), with a deadspace of 0.7 ml and accurate flow measurements in the range of 0.024-30 L/min, was placed at the expiratory limb of the nCPAP system, allowing for the measurement of inspiratory and expiratory flow variation during breathing in all patients.

All tracings were recorded in sync (Figure 1) and analysis was performed off-line using a custom-made software package (Polybench v. 1.25.2, Applied Biosignals, Weener, Germany).

For the selection of the apnea in the present study, 3 investigators scanned the data of all included infants of the caffeine study. First, using only stable tracings of flow, SpO_2 and HR, we identified all recorded cases of apnea, defined as: a cessation of breathing in the flow signal for > 20 s or of shorter duration if accompanied by a hypoxemia (SpO_2 <80%) or bradycardia (a drop in HR to <100 beats/minute).¹ Second, using only the RIP recording (gold standard), apnea was independently classified by the investigators who used the following criteria: 1) central apnea: both the RC and AB tracings were flat lines; 2) obstructive apnea: RC and AB tracings moved in opposite (paradoxical)

directions while the summed RIP signal approached zero; 3) mixed apnea: both central and obstructive components were visible in the RIP tracings. In case of disagreement, the investigators tried to reach consensus about the classification.

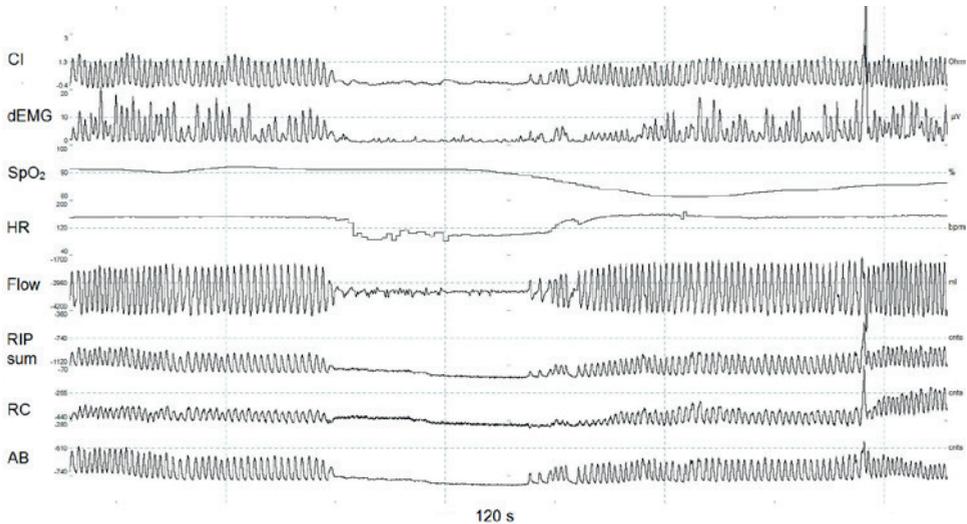


Figure 1. Example of respiratory tracings of dEMG, CI and RIP combined with SpO₂, HR and flow for an apnea classified as central. CI, chest impedance; dEMG, diaphragmatic electromyography; SpO₂, oxygen saturation; HR, heart rate; RIP sum, summed ribcage and abdominal signal of respiratory inductance plethysmography; RC, ribcage; AB, abdominal; cnts, counts; bpm, beats per minute; ml, millilitres; s, seconds.

Forty-nine cases of apnea were identified based on the flow, SpO₂ and HR tracings. Thirty-four of which were classified as central, 5 as obstructive and 10 as mixed apnea according to the RIP tracings. To limit the workload for the assessors classifying the apnea, 15 of the central apnea cases were randomly selected from the total of 34, and these were used for the final analysis.

Next, for each apnea ($n = 30$), the HR and SpO₂ tracing recorded by the Intellivue MP90 monitor, combined with the RR tracing recorded by either CI (Intellivue MP90 monitor) or dEMG was captured in 1 image. As a result, each apnea was captured twice, once using the respiratory tracing based on the CI data, and once based on the dEMG recording. The source of the respiratory tracing (CI or dEMG) was only known to the investigators and was not visible on the image, which was then scored by the assessors. The 60 apnea images were then mixed and e-mailed as a PowerPoint presentation to 22 assessors, consisting of clinical neonatologists ($n = 9$) and paediatricians-in-training ($n = 8$) working in the NICU as well as a random selection of senior nurses with NICU experience ($n = 5$). The assessors were asked to classify each apnea as central, obstructive, or mixed,

based on the respiratory signal, HR and SpO₂ tracings. Basing apnea classification on these 3 tracings is standard procedure in our unit and all health care professionals are trained in apnea classification. For this reasons, no special instructions on how to classify apnea were provided to the assessors.

Statistical analysis

Statistical analysis was performed using SPSS v23 (SPSS, Chicago, Illinois, USA). Descriptive data of the study population were expressed as mean \pm standard deviation (SD). The number of correctly scored apnea in total, and for the dEMG and CI tracings separately, was expressed as a proportion of the total number of scored apnea images (%). Subgroup analyses were performed for the type of apnea and the different assessors. For between-group analysis (dEMG vs. CI), the McNemar test was used. Next, a multivariate logistic regression analysis was performed, correcting the classification of apnea using 1) the type of apnea, 2) the type of assessor, and 3) the type of measurement technique (CI or dEMG) as covariates. A p value < 0.05 was considered statistically significant.

Results

The 30 selected apnea originated from the recordings of 12 preterm infants with a mean GA of 29.0 ± 0.8 weeks and mean birth weight of $1,279 \pm 222$ g. All the included infants were supported by nCPAP and received caffeine. All flow-based apneas detected were also detected by either CI or dEMG. There was no disagreement between the investigators in classifying the apnea as central, obstructive, or mixed, based on the RIP tracing.

Based on the 60 apnea images which were scored by 22 assessors, a total of 1,320 apnea scores were collected and analyzed. In total, 71.1% of all the images were scored correctly as central, obstructive, or mixed (Table 1). Regarding the apneas based on the respiratory tracings of dEMG, 74.8% were classified correctly versus 67.3% of the apnea based on the respiratory tracings of CI. This difference was statistically significant ($p < 0.001$).

Subgroup analyses based on the type of apnea showed that this improvement in apnea classification in favor of dEMG was most prominent in the obstructive apnea subgroup, and, to a lesser extent, in the central apnea subgroup (Table 1). Furthermore, the highest correct rate in total was reached in the central apnea group (83.5%) and the lowest correct rate in the obstructive apnea group (44.5%).

Table 1. Correctly scored apnea in the dEMG and CI groups for classification of apnea

	dEMG	CI	p value
All apnea (<i>n</i> = 1,320)	74.8%	67.3%	<0.001
Central % (<i>n</i> = 660)	86.7%	80.3%	<0.02
Obstructive % (<i>n</i> = 220)	56.4%	32.7%	<0.001
Mixed % (<i>n</i> = 440)	66.4%	65.0%	0.8 (ns)

The *p* value represents the difference between the dEMG and CI group (McNemar test). dEMG, all apnea scored based on the dEMG tracing; CI, all apnea scored based on the CI tracing. *n*, number of images.

Subgroup analysis also showed that the improved apnea classification in the dEMG subgroup compared to the CI subgroup was a finding consistent across the 3 different groups of assessors, even though this was not statistically significant within each subgroup (Table 2). The differences between the groups of assessors regarding correct classification of apnea were small.

Table 2. Correctly scored apnea in the dEMG and CI groups by different assessors

	dEMG (<i>n</i> = 660)	CI (<i>n</i> = 660)	p value
All assessors (<i>n</i> = 22)	74.8%	67.3%	<0.001
Neonatologists (<i>n</i> = 9)	70.7%	65.2%	0.1 (ns)
Paediatricians in training (<i>n</i> = 8)	77.1%	68.3%	<0.02
Nurses (<i>n</i> = 5)	78.7%	69.3%	0.055 (ns)

The *p* value represents the difference between the dEMG and CI group (McNemar test). dEMG, all apnea scored based on the dEMG tracing; CI, all apnea scored based on the CI tracing. *n*, number of images (column heads) and assessors (row heads)

In the multivariate logistic regression analysis, the classification of apnea was still better based on dEMG than based on CI ($p = 0.001$). Furthermore, central apneas were scored better than obstructive and mixed apneas ($p < 0.001$). However, there were no differences in the classification of apnea across the 3 groups of assessors after correction for type of apnea and measurement technique ($p = 0.085$).

Discussion

This study shows that classification of apnea using transcutaneous dEMG is feasible in preterm infants. It also suggests that dEMG might improve apnea classification compared to CI, the current monitoring standard.

There is a growing interest in using the neural activity of the diaphragm for respiratory management of preterm infants. Most studies have reported on the use of

diaphragmatic activity measured by a special transesophageal nasogastric catheter to synchronize invasive and noninvasive respiratory support in preterm infants.^{18,19} Some have suggested that transesophageal dEMG can also be used for assessing breathing patterns and apnea²⁰, but this has so far not been systematically studied. Our study is the first to compare apnea classification according to dEMG to CI. Furthermore, this is the first study to use the noninvasive and cheaper transcutaneous interface.

We used RIP as the gold standard for apnea classification, as previous studies have shown that this technique has no interference from cardiac artefacts, and is especially suitable for distinguishing between central and obstructive apnea.^{1,8,21} However, compared to nasal end-tidal CO₂ or nasal/oral thermistors, the ability of RIP to detect apnea has limitations.²² For this reason, we used a combination of flow, SpO₂ and HR to detect apnea and its consequences, i.e., hypoxemia and bradycardia, from the patients' records.

Consistent with our hypothesis, dEMG monitoring resulted in more accurate classification than CI monitoring in cases of central and obstructive apnea, but not in cases of mixed apnea. It has been suggested that CI has a limited ability to distinguish obstructive apnea from normal respiration.⁸ Although air entry will be limited or absent, air can still move back and forth within the chest wall cavity during airway obstruction, resulting in a normal or slightly reduced breathing pattern when measured with CI; however, respiratory muscle activity is significantly increased during obstructive apnea because the infant is breathing against an occluded airway. The concomitant increase in electrical diaphragmatic activity will be picked up by dEMG monitoring. Therefore, the increase in breathing activity during obstructive apnea is expected to be more accurate when using dEMG monitoring than when using CI. This may explain the improved classification of obstructive apnea with dEMG.

During central apnea, there is a cessation of inspiratory effort and flow, which results in absent electrical activity of the diaphragm and no change in lung aeration. Both dEMG and CI tracings should therefore show no activity (flat line). However, previous reports have shown that cardiac activity may interfere with the CI tracing and (falsely) suggest breathing activity.^{9,11} Such cardiac interference is not present in the dEMG tracing due to a special filtering technique and this may explain the superior classification of central apnea.

A possible explanation why there was no difference between dEMG and CI when classifying mixed apnea is the fact that both central and obstructive components are present in the CI and dEMG tracings. This might make the classification of mixed apnea less dependent on the type of technique (CI or dEMG) for (cardio) respiratory monitoring.

This was the first time that neonatologists, pediatricians-in-training and neonatal nurses assessed respiratory tracings based on dEMG. It seems that the assessors did not have any difficulty interpreting the dEMG tracings; the results of our study show

that the rate of correctly scored apneas based on the dEMG tracings was comparable or better than when based on CI tracings. This finding suggests that dEMG can probably be easily implemented in daily clinical practice. We speculate that classification of apneas will improve even further once assessors are more familiar with interpreting the dEMG tracings.

This study has some limitations that need to be addressed. First, we only assessed a limited number of apneas to keep the workload for each individual assessor within reasonable limits. However, the total number of assessments was 1,320, and we think this is a sufficient number to explore a potential role of dEMG in apnea classification. Second, we only selected apnea from stable RIP, flow, SpO₂ and HR tracings. However, apnea can also occur when tracings are unstable due to, for instance, a patient's movement. It is unclear how dEMG will compare to CI under such circumstances. Finally, we did not measure (absolute) flow directly at the airway opening but at the expiratory limb of the nCPAP system. Although unconventional, the variation in flow did allow us to assess cessation of flow in the respiratory system.

In conclusion, this study shows that electrical activity of the diaphragm measured by transcutaneous dEMG can be used for apnea classification in preterm infants. dEMG improves classification of central and obstructive but not mixed apnea when compared with the current standard, CI, and this finding was consistent across different assessors. These findings suggest that transcutaneous dEMG is a promising candidate for improved analysis of breathing patterns in monitoring systems in the future.

Acknowledgements

We thank all assessors of our department for scoring the apneas and we thank Leo van Eykern and Tom Leenhoven for their technical assistance.

References

1. Sale SM. Neonatal apnoea. *Best Pract Res Clin Anaesthesiol*. 2010 Sep;24(3):323–36.
2. Martin RJ, Abu-Shaweesh JM, Baird TM. Apnoea of prematurity. *Paediatr Respir Rev*. 2004;5:5377–82.
3. Finer NN, Barrington KJ, Hayes BJ, Hugh A. Obstructive, mixed, and central apnea in the neonate: physiologic correlates. *J Pediatr*. 1992 Dec;121(6):943–50.
4. Eichenwald EC. Apnea of Prematurity. *Pediatrics*. 2016;137(1):e20153757.
5. Poets CF, Roberts RS, Schmidt B, Whyte RK, Asztalos EV, Bader D, et al. Association Between Intermittent Hypoxemia or Bradycardia and Late Death or Disability in Extremely Preterm Infants. *Jama*. 2015;314(6):595.
6. Martin RJ, Abu-Shaweesh JM. Control of breathing and neonatal apnea. *Biol Neonate*. 2005 Jan;87(4):288–95.
7. Abu-Shaweesh JM, Martin RJ. Neonatal apnea: what's new? *Pediatr Pulmonol*. 2008 Oct;43(10):937–44.
8. Di Fiore JM. Neonatal cardiorespiratory monitoring techniques. *Semin Neonatol*. 2004;9(3):195–203.
9. Lee H, Rusin CG, Lake DE, Clark MT, Guin L, Smoot TJ, et al. A new algorithm for detecting central apnea in neonates. *Physiol Meas*. 2012;33:1–17.
10. Wilkinson JN, Thanawala VU. Thoracic impedance monitoring of respiratory rate during sedation—is it safe? *Anaesthesia*. 2009 Apr;64(4):455–6.
11. Upton CJ, Milner AD, Stokes GM. Combined impedance and inductance for the detection of apnoea of prematurity. *Early Hum Dev*. 1990 Oct;24(1):55–63.
12. Kraaijenga JV, Hutten GJ, de Jongh FH, van Kaam AH. Transcutaneous electromyography of the diaphragm: A cardio-respiratory monitor for preterm infants. *Pediatr Pulmonol*. 2014;50(9):889–95.
13. Kraaijenga JV, Hutten GJ, de Jongh FH, van Kaam AH. The Effect of Caffeine on Diaphragmatic Activity and Tidal Volume in Preterm Infants. *J Pediatr*. 2015;167(1):70–5.
14. Maarsingh EJ, van Eykern LA, Sprikkelman AB, Hoekstra MO, van Aalderen WM. Respiratory muscle activity measured with a noninvasive EMG technique: technical aspects and reproducibility. *J Appl Physiol*. 2000;88(6):1955–61.
15. O'Brien M, van Eykern L, Precht H. Monitoring respiratory activity in infants - a non-intrusive diaphragm EMG technique. *Non-invasive physiological measurements*. Londen: Academic Press Inc. 1983. p. 131–77.
16. Markhorst DG, Van Gestel JP, van Genderingen HR, Haitzma JJ, Lachmann B, van Vught AJ. Respiratory inductive plethysmography accuracy at varying PEEP levels and degrees of acute lung injury. *J Med Eng Technol*. 2006;30(3):166–75.
17. Valta P, Takala J, Foster R, Weissman C, Kinney JM. Evaluation of respiratory inductive plethysmography in the measurement of breathing pattern and PEEP-induced changes in lung volume. *Chest*. 1992;102(1):234–8.
18. Stein H, Beck J, Dunn M. Non-invasive ventilation with neurally adjusted ventilatory assist in newborns. *Semin Fetal Neonatal Med*. 2016;21(3):154–61.
19. Beck J, Reilly M, Grasselli G, Mirabella L, Slutsky AS, Dunn MS, et al. Patient-ventilator interaction during neurally adjusted ventilatory assist in low birth weight infants. *Pediatr Res*. 2009;65(6):663–8.

20. Ng E, Schurr P, Reilly M, Dunn M, Beck J. Impact of feeding method on diaphragm electrical activity and central apnea in preterm infants (FEAdi study). *Early Hum Dev.* 2016;101:33–7.
21. Brouillette RT, Morrow AS, Weese-Mayer DE, Hunt CE. Comparison of respiratory inductive plethysmography and thoracic impedance for apnea monitoring. *J Pediatr.* 1987 Sep;111(3):377–83.
22. Weese-Mayer DE, Corwin MJ, Peucker MR, Di Fiore JM, Hufford DR, Tinsley LR, et al. Comparison of apnea identified by respiratory inductance plethysmography with that detected by end-tidal CO₂ or thermistor. *Am J Respir Crit Care Med.* 2000;162(2 1):471–80.